


A WHITE PAPER

The Benefits of Light and Dark Pixel Thresholding

WHAT IS THRESHOLDING?

Thresholding is a method of image segmentation used in image processing to discern the boundaries of an object from its background. Semi-transparent particles, such as protein aggregates, are often mischaracterized or even undetected by most imaging particle analyzers when thresholding is missing or improperly configured.

Dark pixel thresholding, offered by most imaging particle analyzers, fails to discern particulate matter when it is lighter than the imaged background. Utilization of both dark and light pixel thresholding enables the detection and discernment of particulates expressing ranges in opacity (opaque to transparent) and improves the particle analyzer's ability to detect, image, and analyze semi-transparent particles.

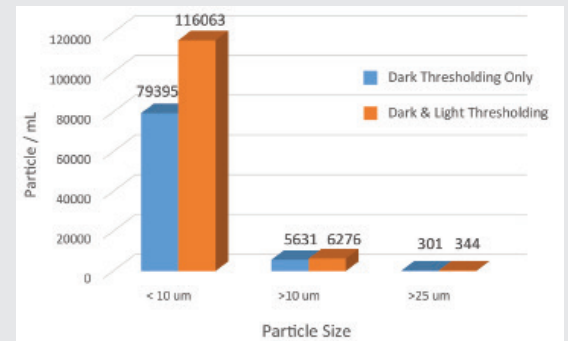

A protein sample was analyzed using dark pixel thresholding and both dark and light pixel thresholding. Utilization of dark and light thresholding showed an increase in particle count in all size bins. Learn how the FlowCam uses light and dark thresholding at www.fluidimaging.com/resources/tech-briefs

HOW DOES THRESHOLDING AFFECT INSTRUMENT SENSITIVITY?

Thresholding uses pixel intensities to differentiate the boundaries of the object from its background. Each pixel in the grayscale image is assigned an intensity value from 0 (black) to 255 (white). Color images are converted to grayscale images prior to intensity assignments. The intensity of each pixel in the image is compared to the background pixel intensity and the thresholding value. Based on these comparisons, the pixel is determined to be part of either the foreground object or the background. Dark pixel thresholding recognizes objects with pixel intensities darker than the background. Light and dark pixel thresholding recognizes objects with pixel intensities lighter and/or darker than their background. This is ideal for transparent/semi-transparent particles such as protein aggregates.


In most particle analyzers, opaque particles are darker than their background as viewed by the camera because the illumination source is located behind the flow cell. For this reason, most imaging particle analyzers use dark pixel thresholding only. However, dark pixel thresholding of semi-transparent particles, such as protein aggregates, often leads to fractionation into several smaller particles which results in inaccurate physical measurements and particle count. Use of both dark and light pixel thresholding during particle analysis recognizes the grayscale range (opaque to transparent) of semi-transparent particles, reduces fractionation, and improves particle count and morphological characterization.

The Benefits of Light and Dark Pixel Thresholding

THE BENEFIT OF DUAL THRESHOLDING


1. Raw Image

No detection




2. Dark Threshold Only

Using 25 Grey intensity levels
(3 medium/35 small particles)




3. Dark Threshold Only

15 Grey intensity levels
More large particles
detected than previous
(6 medium/8 small)




4. Light Threshold Only

15 Grey intensity levels
(4 Medium/42 small particles)




5. Dark and Light Threshold

Both 15 Grey intensity levels
(1 large/28 small)



6. Dark Threshold and Light Threshold -

Both 15 Grey intensity levels
+ VisualSpreadsheet
(One large particle – best characterization of
this protein)



The figure above illustrates particle analysis of a semi-transparent particle using various threshold settings. These images were obtained using the FlowCam particle analyzer, which has dark and/or light pixel thresholding capabilities. Each green box delineates a separate particle, as identified by the FlowCam's analysis software VisualSpreadsheet, and portions identified as part of each particle are colored red.

The use of only one pixel setting (either light or dark) resulted in the fractionation of the protein aggregate into as many as 46 separate particles. As image 1 shows, the protein aggregate analyzed was comprised of portions darker and lighter than the image background. When dark pixel thresholding was used, only the portions of the protein darker than the background were recognized as particulate matter, and the protein was falsely subdivided into several smaller particles (images 2 and 3). When light pixel thresholding was used, only portions of the particle lighter than the background were recognized as particulate matter and the protein was also falsely subdivided into several smaller particles (image 4). Changes in opacity of the protein aggregate result in changes in grayscale intensity. The application of only a single type of pixel thresholding (dark or light) failed to accurately analyze a particle exhibiting both light and dark portions.

The use of both dark and light pixel settings, in conjunction with VisualSpreadsheet's neighborhood analysis feature, resulted in accurate particle characterization of the protein aggregate. When dark and light pixel thresholding was used, the particle analyzer recognized both dark and light portions of the particle as particulate matter. The filamentous nature of this protein, however, resulted in minor fractionation of the aggregate (image 5). When the software's neighborhood analysis was applied, the whole protein (both light and dark portions) was recognized as a single particle (image 6).

Dark and light pixel thresholding and VisualSpreadsheet's neighborhood analysis are necessary to accurately analyze semi-transparent particles. Read Fluid Imaging Technologies' Technical Brief to learn how to modify threshold settings on the FlowCam, use VisualSpreadsheet, and optimize analysis of any particulate matter at www.fluidimaging.com/resources/tech-briefs.